


Figure S2. Bland-Altman Plots between wearable and ambulatory blood pressure monitoring devices (24-hours).

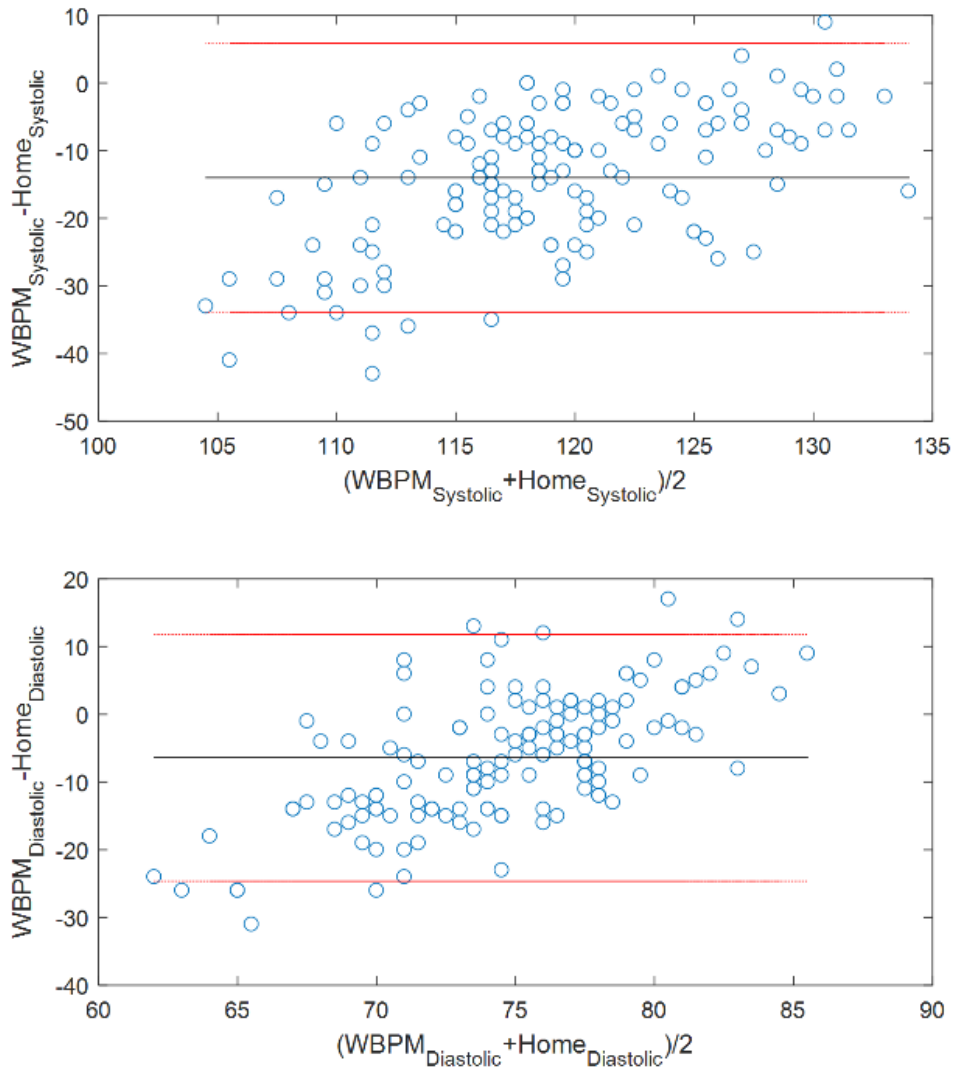

Measurement uncertainty during 24 hours of concurrent ambulatory (ABPM) and wearable (WBPM) blood pressure monitoring. Black reference line = mean bias, red reference lines = 95% limits of agreement.